



**FWT-60-00 Batch Characterization**  
**Batch 1155**

**Typical Calibration Curve**


(Dosimeters pre-conditioned to 20 °C and 50%RH)

Dose, kGy	k, mm <sup>-1</sup> at 605 nm	k, mm <sup>-1</sup> at 600 nm	k, mm <sup>-1</sup> at 510 nm
1	1.74	1.71	
5	8.21	8.01	0.97
10	15.79	15.40	1.85
30	40.18	39.30	4.83
50	56.97	56.12	7.25
70			9.31
100			11.87
150			15.03
200			17.09

**Coefficient of Variation of k**

605 nm	600 nm	510 nm
1.6%	1.5%	2.2%

Note: k is the specific absorbance and is determined from the thickness, t, and final and initial absorbances Af and Ai:  
 $k = (A_f - A_i) / t$ .

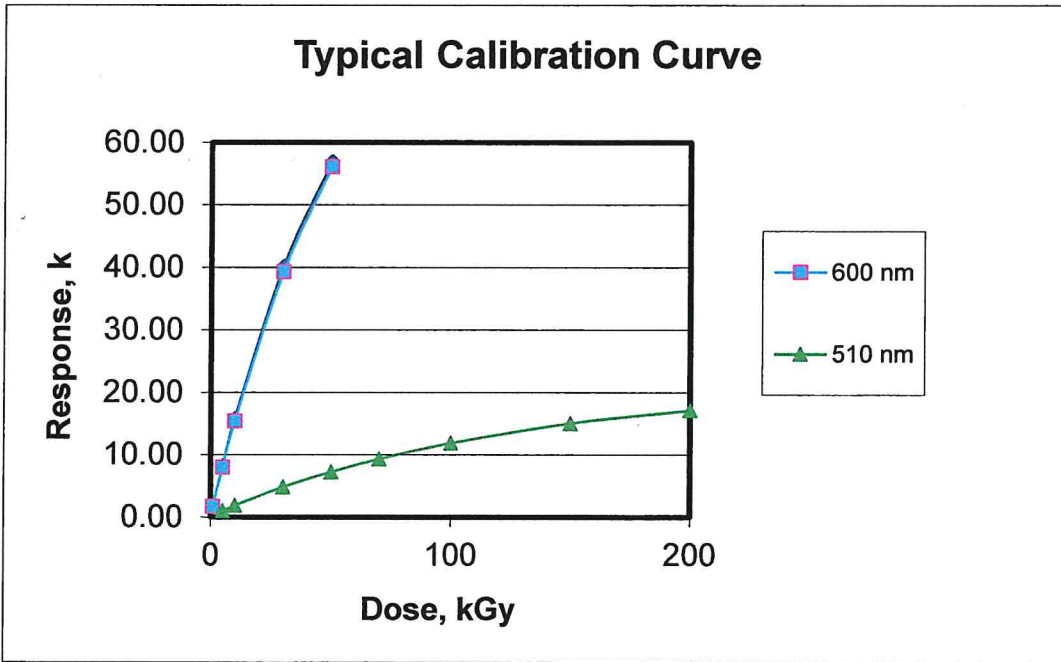

This typical calibration curve is provided as a guide to the response of FWT-60-00 Radiachromic Detectors to ionizing radiation. Actual response also depends on processing parameters and on the instrumentation used to measure absorbancies and thicknesses.

Scott Larson  
Authorization for Release

January 25, 2019  
Date



## FWT-60-00 Batch Characterization


### Batch 1155

#### Temperature Dependence

(Dosimeters pre-conditioned to 20 °C and 50%RH)

T, °C	k, mm <sup>-1</sup> at 605 nm	k, mm <sup>-1</sup> at 600 nm	k, mm <sup>-1</sup> at 510 nm
-75	27.60	26.88	3.26
-50	30.08	29.31	3.55
-25	31.35	30.57	3.74
0	33.76	32.96	4.14
20	35.39	34.58	4.23
30	35.20	34.38	4.21
40	35.09	34.29	4.20
50	35.77	34.96	4.27

T, °C	Norm. k at 605 nm	Norm k at 600 nm	Norm k at 510 nm
-75	0.82	0.82	0.79
-50	0.89	0.89	0.86
-25	0.93	0.93	0.90
0	1.00	1.00	1.00
20	1.05	1.05	1.02
30	1.04	1.04	1.02
40	1.04	1.04	1.02
50	1.06	1.06	1.03

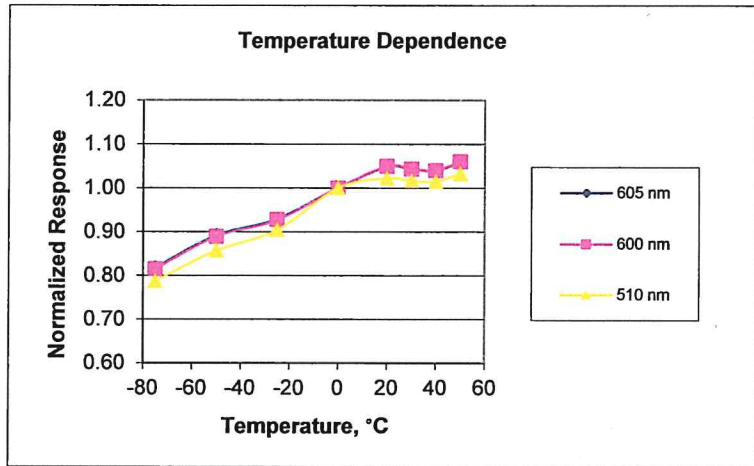

#### Humidity Dependence

(Dosimeters pre-conditioned to the indicated humidity at 20 °C)

%RH	k, mm <sup>-1</sup> at 605 nm	k, mm <sup>-1</sup> at 600 nm	k, mm <sup>-1</sup> at 510 nm
30	40.90	40.07	5.08
40	40.94	40.10	4.97
45	40.49	39.64	4.88
50	39.67	38.83	4.77
55	38.87	38.03	4.64
60	37.40	36.58	4.47

%RH	Norm. k at 605 nm	Norm k at 600 nm	Norm k at 510 nm
30	1.03	1.03	1.06
40	1.03	1.03	1.04
45	1.02	1.02	1.02
50	1.00	1.00	1.00
55	0.98	0.98	0.97
60	0.94	0.94	0.94

