



Tel: +1.805.964.3615 info@fwt.com
 Fax: +1.805.964.3162 www.fwt.com
 330 Kellogg Avenue, Suite D, Goleta, CA 93117 U.S.A.

FWT-60-00 Batch Characterization

Batch 1147

Typical Calibration Curve


(Dosimeters pre-conditioned to 20 °C and 50%RH)

Dose, kGy	k, mm ⁻¹ at 605 nm	k, mm ⁻¹ at 600 nm	k, mm ⁻¹ at 510 nm
1	1.88	1.84	
5	8.48	8.31	1.01
10	15.83	15.53	1.89
30	40.99	40.33	5.02
50	57.70	57.09	7.55
70			9.65
100			11.88
150			14.84
200			16.99

Coefficient of Variation of k

605 nm	600 nm	510 nm
2.6%	2.6%	3.6%

Note: k is the specific absorbance and is determined from the thickness, t, and final and initial absorbances Af and Ai:
 $k = (A_f - A_i) / t$

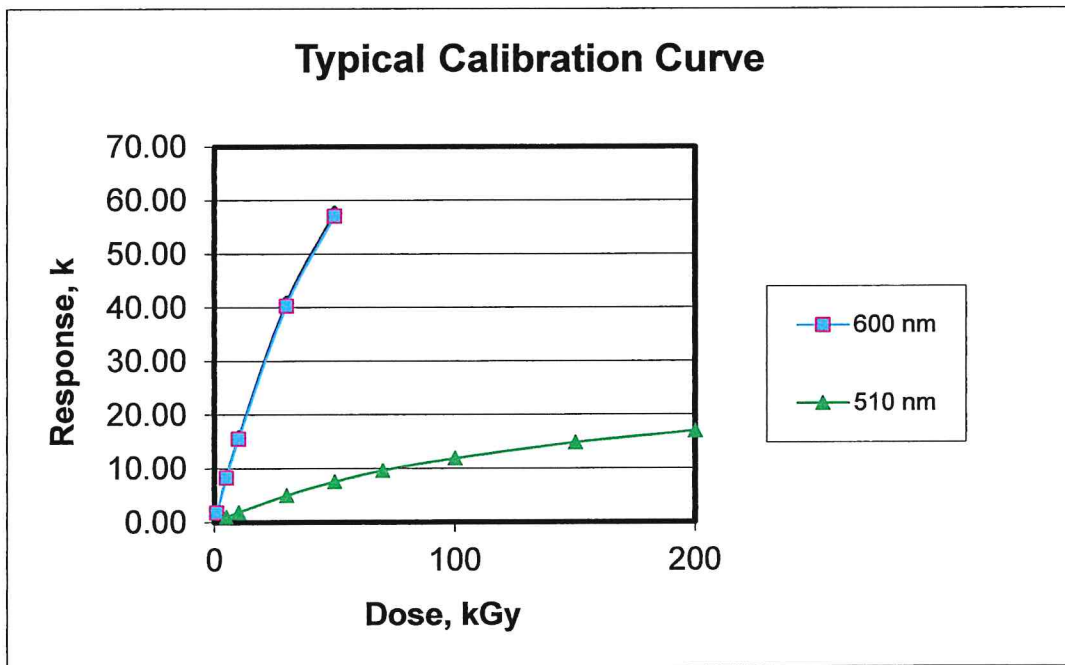

This typical calibration curve is provided as a guide to the response of FWT-60-00 Radiachromic Detectors to ionizing radiation. Actual response also depends on processing parameters and on the instrumentation used to measure absorbancies and thicknesses.

Scott A. Larson
 Authorization for Release

22 November 2017
 Date



Tel: +1.805.964.3615 info@fwt.com
 Fax: +1.805.964.3162 www.fwt.com
 330 Kellogg Avenue, Suite D, Goleta, CA 93117 U.S.A.

FWT-60-00 Batch Characterization


Batch 1147

Temperature Dependence

(Dosimeters pre-conditioned to 20 °C and 50%RH)

T, °C	k, mm ⁻¹ at 605 nm	k, mm ⁻¹ at 600 nm	k, mm ⁻¹ at 510 nm
-75	29.08	28.50	3.56
-50	31.91	31.26	3.85
-25	32.12	31.50	3.92
0	34.81	34.16	4.36
20	36.57	35.92	4.47
30	36.68	36.04	4.50
40	36.59	35.95	4.50
50	36.71	36.06	4.54

T, °C	Norm. k at 605 nm	Norm k at 600 nm	Norm k at 510 nm
-75	0.84	0.83	0.81
-50	0.92	0.92	0.88
-25	0.92	0.92	0.90
0	1.00	1.00	1.00
20	1.05	1.05	1.02
30	1.05	1.05	1.03
40	1.05	1.05	1.03
50	1.05	1.06	1.04

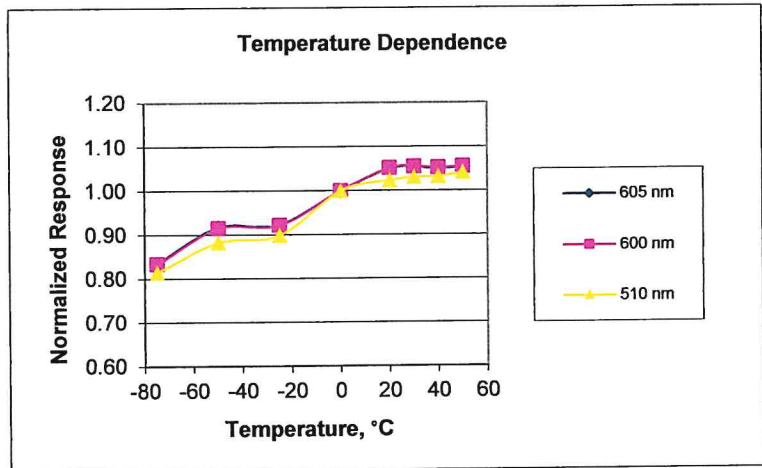

Humidity Dependence

(Dosimeters pre-conditioned to the indicated humidity at 20 °C)

%RH	k, mm ⁻¹ at 605 nm	k, mm ⁻¹ at 600 nm	k, mm ⁻¹ at 510 nm
30	42.36	41.68	5.40
40	43.62	42.95	5.44
45	42.09	41.40	5.20
50	41.49	40.79	5.11
55	40.47	39.78	4.99
60	39.32	38.66	4.99

%RH	Norm. k at 605 nm	Norm k at 600 nm	Norm k at 510 nm
30	1.02	1.02	1.06
40	1.05	1.05	1.06
45	1.01	1.01	1.02
50	1.00	1.00	1.00
55	0.98	0.98	0.98
60	0.95	0.95	0.98

